



Sunset
Laboratory Inc.

Sunset Laboratory Model 4 Semi-Continuous OCEC Field Analyzer

- ✓ Organic Carbon
- ✓ Elemental Carbon
- ✓ Black Carbon
- ✓ Total Carbon



Notice


For further details about the Model 4 OC-EC please contact us or one of our local representatives.

Contact details can be found on the Partners page of our web-site or we may be contacted directly.



Scan the QR code
to visit our website

The Model 4 is the only U.S. EPA ETV verified Black Carbon Monitor (REPORT: EPA/600/R-14/308)

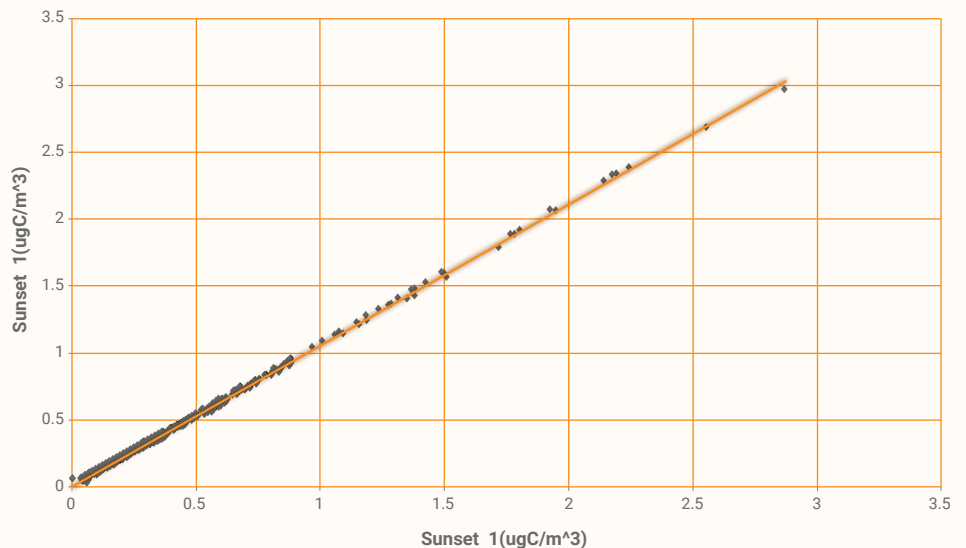

*****Results verified by US-EPA ETV Testing to be equivalent to US-EPA Reference Method (less than +4%)**

Model 4 OCEC Instrument Specifications

Physical dimensions

1. 17" x 15" x 10.5" Standard Rack mount cabinet
2. Wt; approximately 35 pounds

Power Requirements


120 VAC/15 A or 220VAC/8A (Must specify at time of order)

Instrument Package Includes

- Model 4G OCEC Instrument
- Latest Version of Operation & Calculation Software
- Parallel plate denuder
- Sampling pump
- 2.5 μm sharp cut cyclone
- Sample Inlet Installation Kit
- Controlling Laptop Computer w/ Windows 10 Professional, Operation and Calculation Software

Performance Characteristics – real time, semi-continuous operation with typical time resolution from 30 minutes to 24 hours

1. 8 LPM sample rate typical
2. Sample analysis time; 6 – 20 minutes depending on analysis method
3. Time resolution; depends on requirements, but 1 hour is typical for a single instrument application (80% or better sampling duty cycle)
4. Sensitivity and Detection Limit (LDL):
 1. Range: TC - 0.2 to 600 $\mu\text{g}/\text{cm}^2$
 2. Range: OC - 0.2 to 600 $\mu\text{g}/\text{cm}^2$
 3. Range: EC - 0.2 to 30 $\mu\text{g}/\text{cm}^2$
 4. Range: BC (ie. Opt_EC) - 0.05 to 30 $\mu\text{g}/\text{cm}^2$
 5. Limit of Detection - 0.10 $\mu\text{g}/\text{cm}^2$
 6. Limit of Detection for BC - 0.05 $\mu\text{g}/\text{cm}^2$

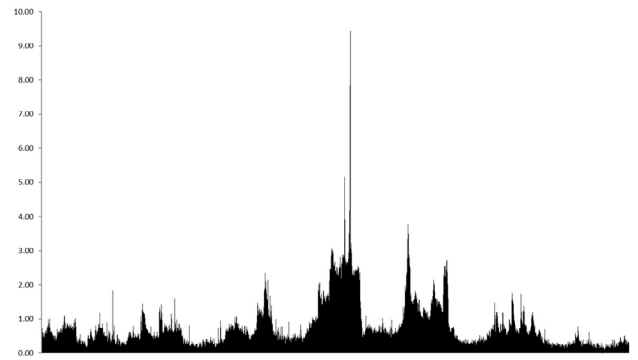

5. Measurement Range:

1. Range for 2 Hour Sample Cycle: OC - 0.2 to 100 $\mu\text{g}/\text{M}^3$
2. Range for 2 Hour Sample Cycle: EC - 0.1 to 20 $\mu\text{g}/\text{M}^3$
3. Range for 2 Hour Sample Cycle: BC - 0.06 to 34 $\mu\text{g}/\text{M}^3$
4. Limit of Detection for 2 Hour Sample Cycle: OC - 0.2 $\mu\text{g}/\text{M}^3$
5. Limit of Detection for 2 Hour Sample Cycle: EC - 0.1 $\mu\text{g}/\text{M}^3$
6. Limit of Detection for 2 Hour Sample Cycle: BC - 0.06 $\mu\text{g}/\text{M}^3$

Measurement Method (User Configurable)


1. NIOSH 5040
2. EUSAAR2
3. Fast TOC with optical EC (BC)
4. IMPROVE-A temperature profile using TO/Transmission
5. User defined custom applications

Calibration

1. External Standard – Uses an external standard calibration gas. A fixed-loop volume of this gas is injected at the end of every analysis. All calculated results are referenced against this external standard.
2. Primary calibrations are referenced against sucrose solutions or NIST traceable gas standards. NIST traceable gas standards are USER provided and must be ordered separately if desired.

Support Gases to be supplied by customer:

1. He (99.999% or better) – Hydrocarbon and CO₂ < 1 ppm
2. 5% methane in Helium Balance – He (99.999%), Methane CP grade, certification to 2%.
3. 10% Oxygen in Helium Balance – (99.999% or better for both gases)

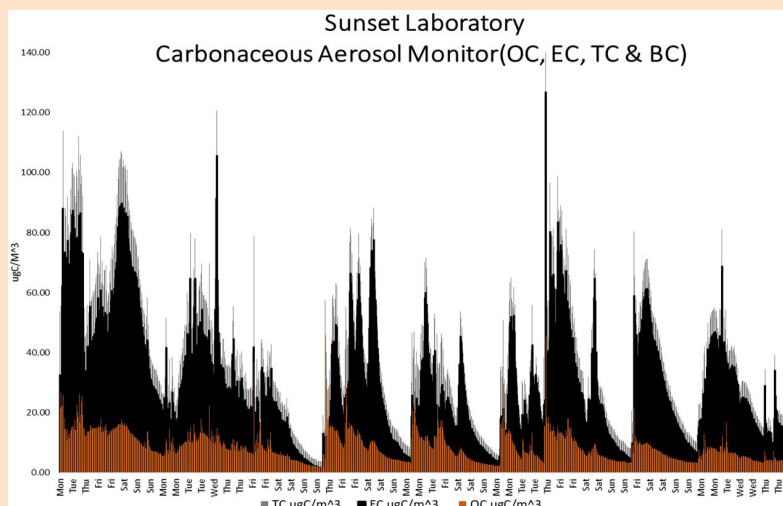

MAIN OFFICE AND SALES

10180 SW Nimbus Avenue - Suite J/5
Tigard, OR US 97223-4341 - United States - 503.624.1100

EAST COAST OFFICE

620-G Valley Forge Road
Hillsborough - NC 27278 - United States - 919.245.3131

WESTERN EUROPEAN OFFICE

Sunset Laboratory B.V. - Science Park 106 - Amsterdam
North Holland - 1098XG The Netherlands - +31 20 70 52 300